



MARSTM
BIO-MED PROCESSES INC

LibertyBOSS STARTER KIT

Upgrade to **NO Maintenance, NO Filters** and **Guaranteed Compliance** for up to 3 years

"We are very pleased with our new LibertyBOSS amalgam separator. Before the BOSS, our suctions were extremely weak. Often, our pump would make loud unpleasant sounds. Since we switched, we do not hear any sounds, and our evacuation lines are consistently powerful."
- Newmarket Health Dental



AMALGAM SEPARATOR STARTER KIT

The Starter Kit includes the following:

- NO maintenance, NO filters, NO inspections for up to 3 years with MARS LibertyBOSS
- All the parts needed for a standard amalgam separator installation
- Amalgam Separator Disposal
- Certificate of Compliance
- Automatic Compliance Reminder
- A Revenue Generating Program:
FREE Advertising as an "Environmentally Friendly Dental Practice"

"In the past, I had the MARS LibertyBOSS. About a year and a half ago, on the advice of a Technician, I changed over to the SolmeteX Hg5. I soon realized that I was having to change the filters every 4 months. Needless to say it was getting expensive. I am happy to come back to MARS, as I don't have to worry about changing the LibertyBOSS for another 3 years. It is good to be a part of the MARS Family of Environmentally Friendly Dental Practices again." - Dr. Anna Shieh, Bronte Dental

CONTACT US

Toll-free: Canada and U.S.A. 1-866-594-3648

Canada:

Head Office

1801 Wentworth St., Unit 1

Whitby, Ontario, L1N 8M2

☎ 905-723-9610

@ info@marsbiomed.com


ARE YOU READY TO UPGRADE TO THE MARS *Liberty***BOSS**?

www.marsbiomed.com



MARS[™]
BIO-MED PROCESSES INC

EPA REGULATION COMPLIANCE FLOW-CHART

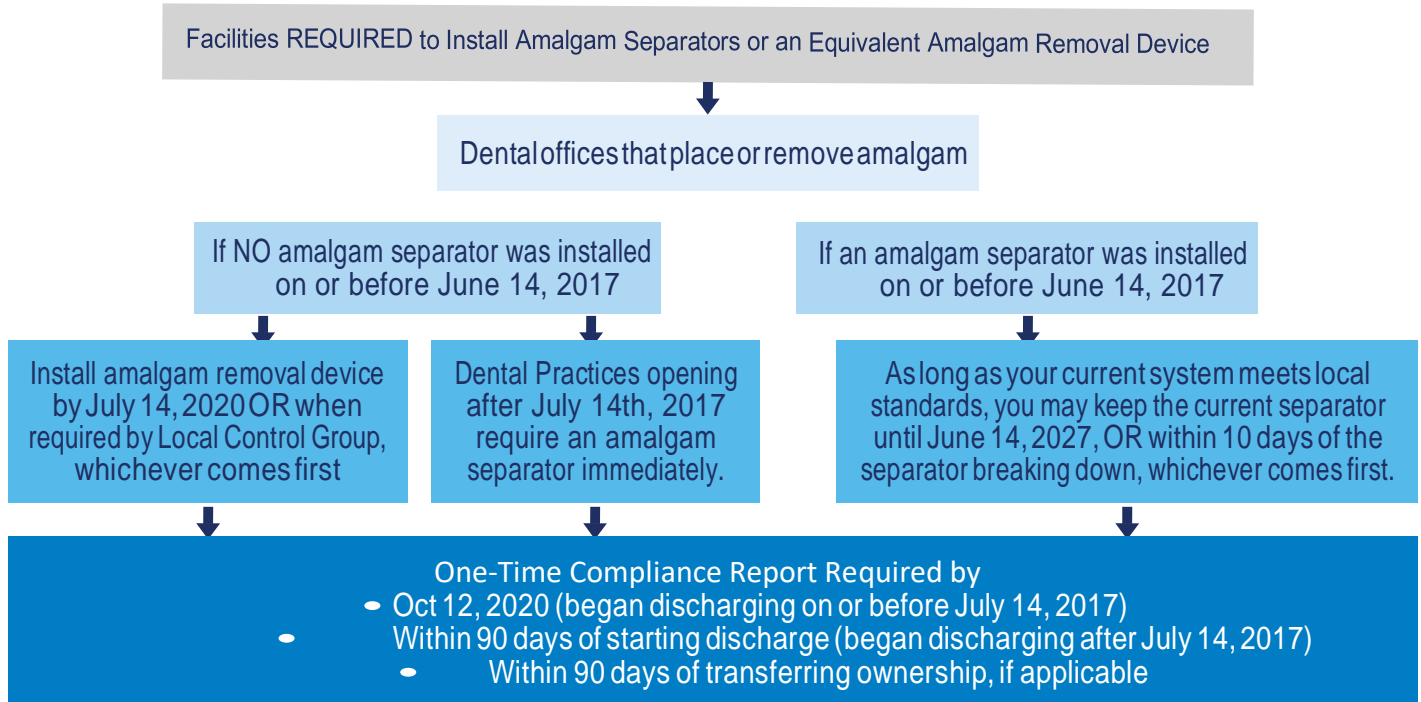

Installed amalgam removal devices must comply with the following Best Management Practices:

1. Keep One-Time Compliance Report on Record for lifetime of ownership
2. Monitor system according to manufacturer's recommendation
3. Maintain by replacing amalgam retaining cartridge, separator, canister or units as directed by manufacturer OR when the amalgam separator stops performing at the system's specified efficiency, whichever comes first.
4. Do not use oxidizing or acidic cleaners (pH < 6 or pH > 8) on dental unit water lines, chair-side traps and vacuum lines.

Must Maintain Records on Site for 3 years of:

- Any reports filed
- A visual inspection log (If required by manufacturer)
- Documentation of any repair or replacement (Cartridges/Filters, etc.)
- Disposal Records
- Certificate of Compliance (If supplied by manufacturer)
- Manufacturer's current operating manual for the device in place.

To Ensure Compliance, Invest in Best Available Technology

"The MARS LibertyBOSS is the only unit that is capable of removing both solid and dissolved mercury from the environment. Their design provides the highest removal rate under normal operating parameters and treats both the total and dissolved mercury."

Conclusion of the Purves Environmental "Dental Separator Study" (2014)

*Visit marsbiomed.com for the full study